


MAR 04 2011

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

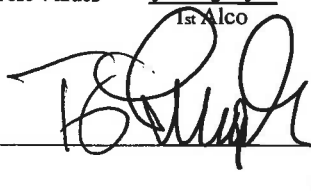Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130292 ✓
Name	TRACY MORPHY	ID#	7252 ✓
Agency	JONKAD Police Dept.	Date	3-1-11 ✓
Instrument Location	JONKAD Police Dept	Phone #	907.586-0000
Alco S/N		Target Value	High Pressure
X172933		1078 ✓	30.48
Alco Test Values		1st Alco	2nd Alco
		1084 ✓	1083 ✓
Signature			
(OVER)			


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 31 day of MAR, 2011.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

MARCH 01, 2011

OPERATOR'S NAME:

MURPHY/TRACY/ERNEST

OPERATOR'S NUMBER: 7252

SUBJECT'S LAST NAME:

MURPHY

SUBJECT'S FIRST NAME/MI :

TRACY

O.L. #: VOC

DEPT/AGENCY: JNU1

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: X172933

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.48 in		
ALCO TARGET	.079	09:41
BLANK TEST	.000	09:42
INTERNAL STANDARD	VERIFIED	09:42
ALCO TV 30.48 in	.084	09:42
BLANK TEST	.000	09:43
SUBJECT SAMPLE	.000	09:44
BLANK TEST	.000	09:44
ALCO TV 30.48 in	.083	09:45
BLANK TEST	.000	09:45

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

MARCH 01, 2011

TIME 09:39

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	41c
BAROMETER:	30.48 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGH
IJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz
~{|}~